

CPEC200's EC155 Gas Analyzer's Packing Information

When the CPEC200 is shipped, the EC155 Gas Analyzer and associated equipment are placed in a foam cutout that helps protect them from damage during shipment. The EC155 should look like the photograph below. After unpacking, it is recommended to save the foam cutout as the EC155 components should be placed in the foam cutout whenever the EC155 is transported to another location.

Note: Another box containing the Sonic Head and its components will also be shipped with the EC155 analyzer if Sensing Head Option –SH has been ordered.

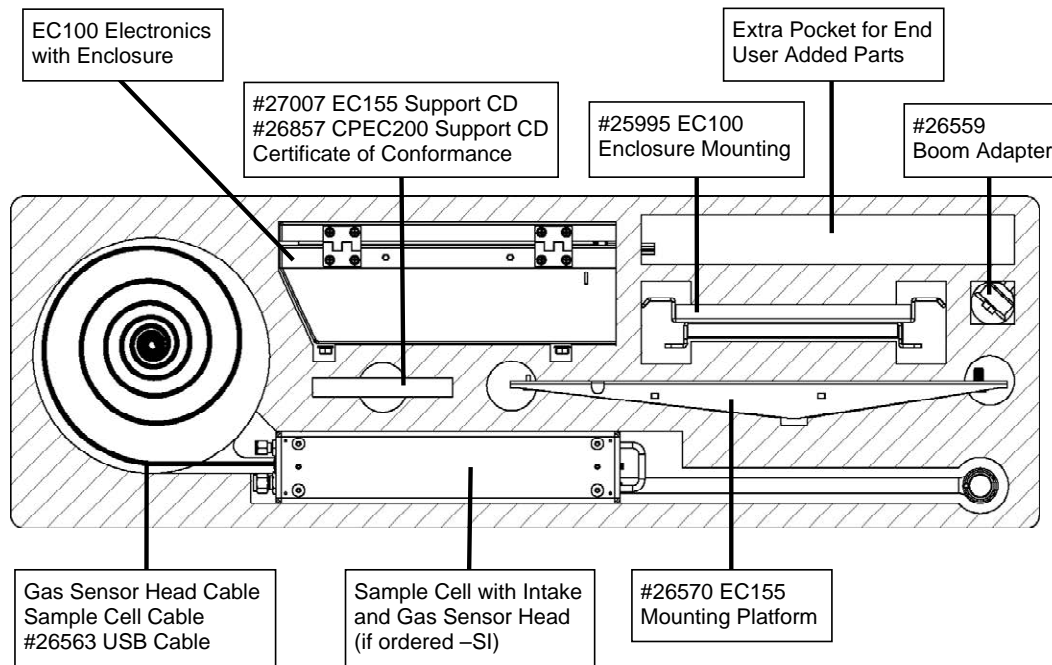


FIGURE 1. CPEC200 with Sample Cell Option -SI

