

# Barometric Pressure Sensor

## Model CS105

The CS105 Barometer uses Vaisala's silicon capacitive sensor to measure barometric pressure over a 600 to 1060 millibar range. The CS105 outputs a linear signal of 0 to 2.5 Vdc allowing it to be directly connected to Campbell Scientific dataloggers.

An integral circuit switches 12 volts from the datalogger to the barometer only during measurement, thereby reducing power requirements. Sensor warm-up and measurement time is one second minimum.


### Construction and Mounting

The sensor is housed in an anodized aluminum case fitted with an intake valve for pressure equilibration. Terminal strips provide for datalogger power and signal connections. The barometer is supplied with 2.5' of cable and is intended to mount inside the ENC 12/14 or larger enclosure.


### Manufacturer's Specifications

- Total Accuracy<sup>1</sup>:  $\pm 0.5$  mb @ +20°C  
 $\pm 1.5$  mb @ 0° to 40°C  
 $\pm 2.0$  mb @ -20° to +45°C  
 $\pm 3.0$  mb @ -40° to +60°C
- Linearity:  $\pm 0.45$  mb
- Hysteresis:  $\pm 0.05$  mb
- Repeatability:  $\pm 0.05$  mb
- Calibration Uncertainty:  $\pm 0.15$  mb
- Long-Term Stability:  $\pm 0.1$  mb per year
- Operating Temperature: -40° to +60° C
- Dimensions: 3.8" x 2.4" x 0.9"  
(9.7 cm x 6.0 cm x 2.2 cm)
- Weight: 3.0 oz (85 g)  
Shipping: 4.1 oz (115 g)
- Supply Voltage: 10 to 30 Vdc
- Current Consumption: <4 mA (active)  
<1  $\mu$ A (quiescent)
- Warm-up Time: 1 s

<sup>1</sup>The root sum squared (RSS) of end point non-linearity, hysteresis, repeatability, and calibration uncertainty.

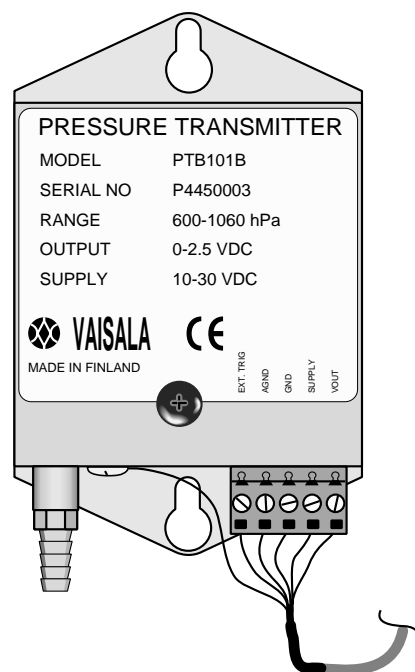

*The CS105 provides accurate, unattended measurements of barometric pressure over a wide range of elevations.*

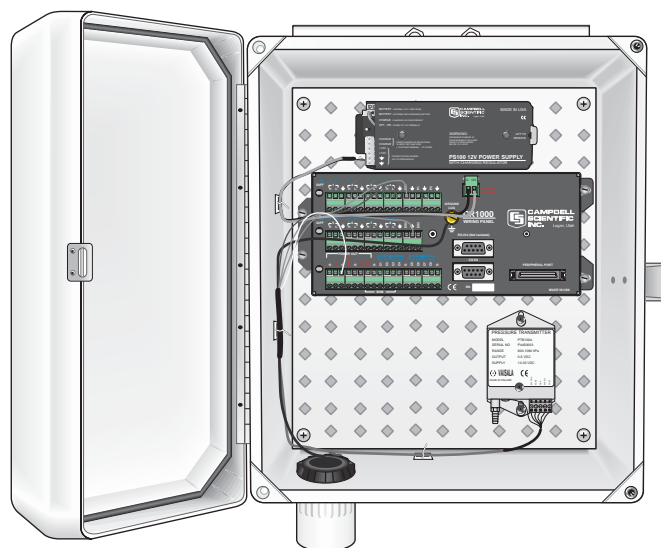

*PS100 12 Vdc power supply top, CR1000 datalogger, and CS105 inside ENC12/14 enclosure.*



**CAMPBELL SCIENTIFIC, INC.**

815 W. 1800 N. • Logan, Utah 84321-1784 • (435) 753-2342 • FAX (435) 750-9540  
Offices also located in: Australia • Brazil • Canada • England • France • South Africa • Spain

Copyright © 1991, 2005  
Campbell Scientific, Inc.  
Printed October 2005